




# Multi-probe Data Storage

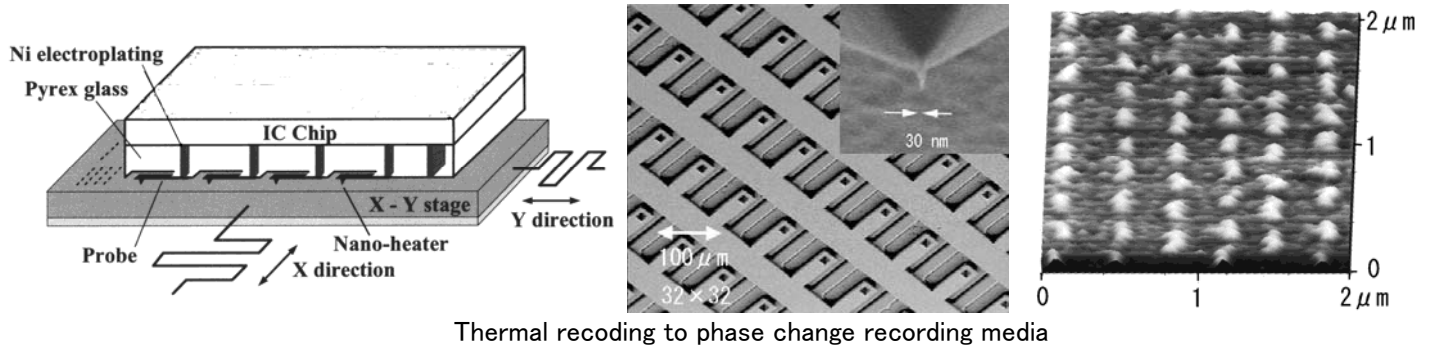

Reference : D.W.Lee, T.Ono, T.Abe and M.Esashi, Microprobe Array with Electrical Interconnection for Thermal Imaging and Data Storage, J. of Microelectromechanical Systems, 11 (2002) pp.215-219

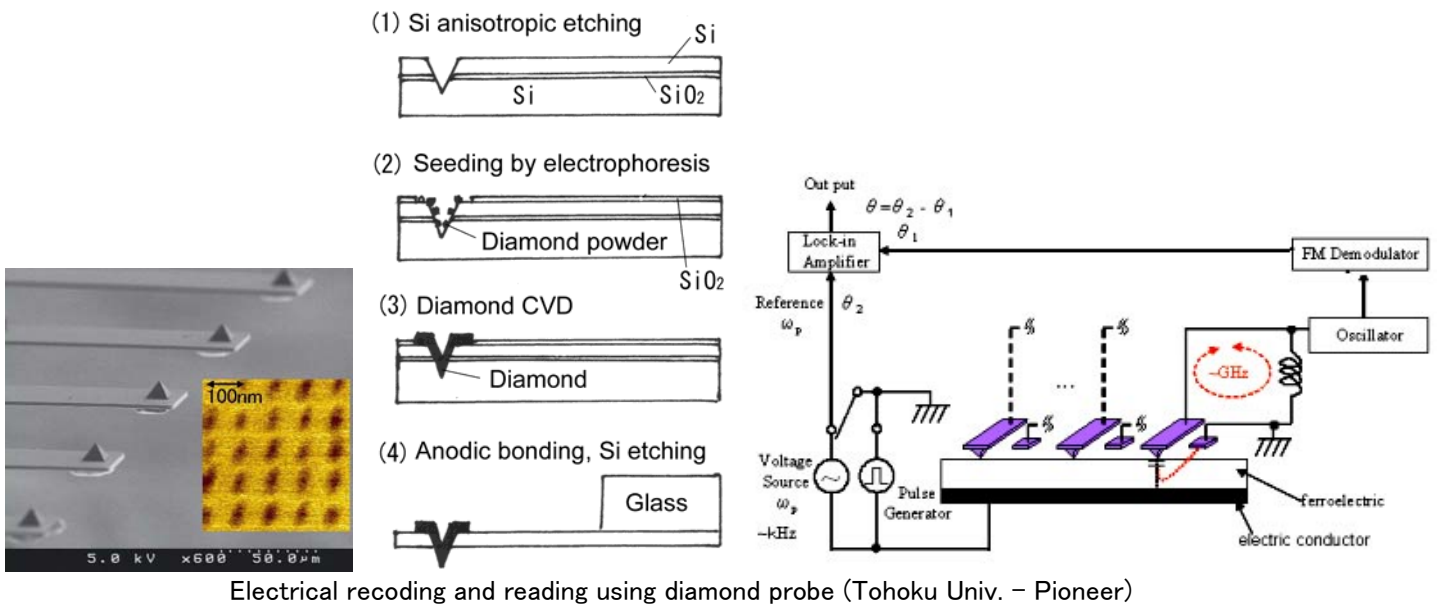

Reference : H.Takahashi, A.Onoe, T.Ono, Y.Cho and M.Esashi, High-Density Ferroelectric Recording Using Diamond Probe by Scanning Nonlinear Dielectric Microscopy, Jap. J. of Applied Physics. 45 (2006) pp.1530-1533

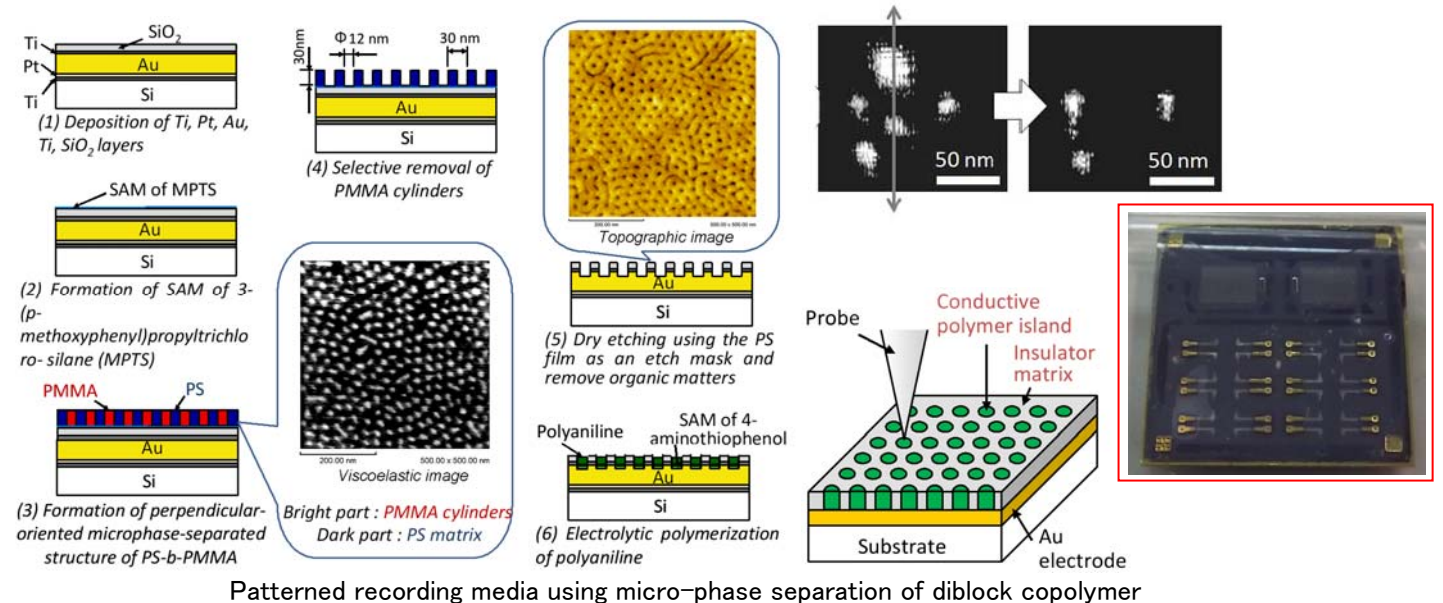

Reference : S.Yoshida, T.Ono and M.Esashi, Conductive Polymer Patterned Media for Scanning Multiprobe Data Storage, Nanotechnology, 18 (2007) 505302(5pp)